


-15kV TOF: -9181 v
 -3.6kV MCP: -3379 v
 -2.4kV MCP: -1774 v
 Input Cur: 300 ma
 RPA max: 237 v
 Mirror max: 238 v

Wed Nov 29 10:38:44 2006

TIDE Direct Events

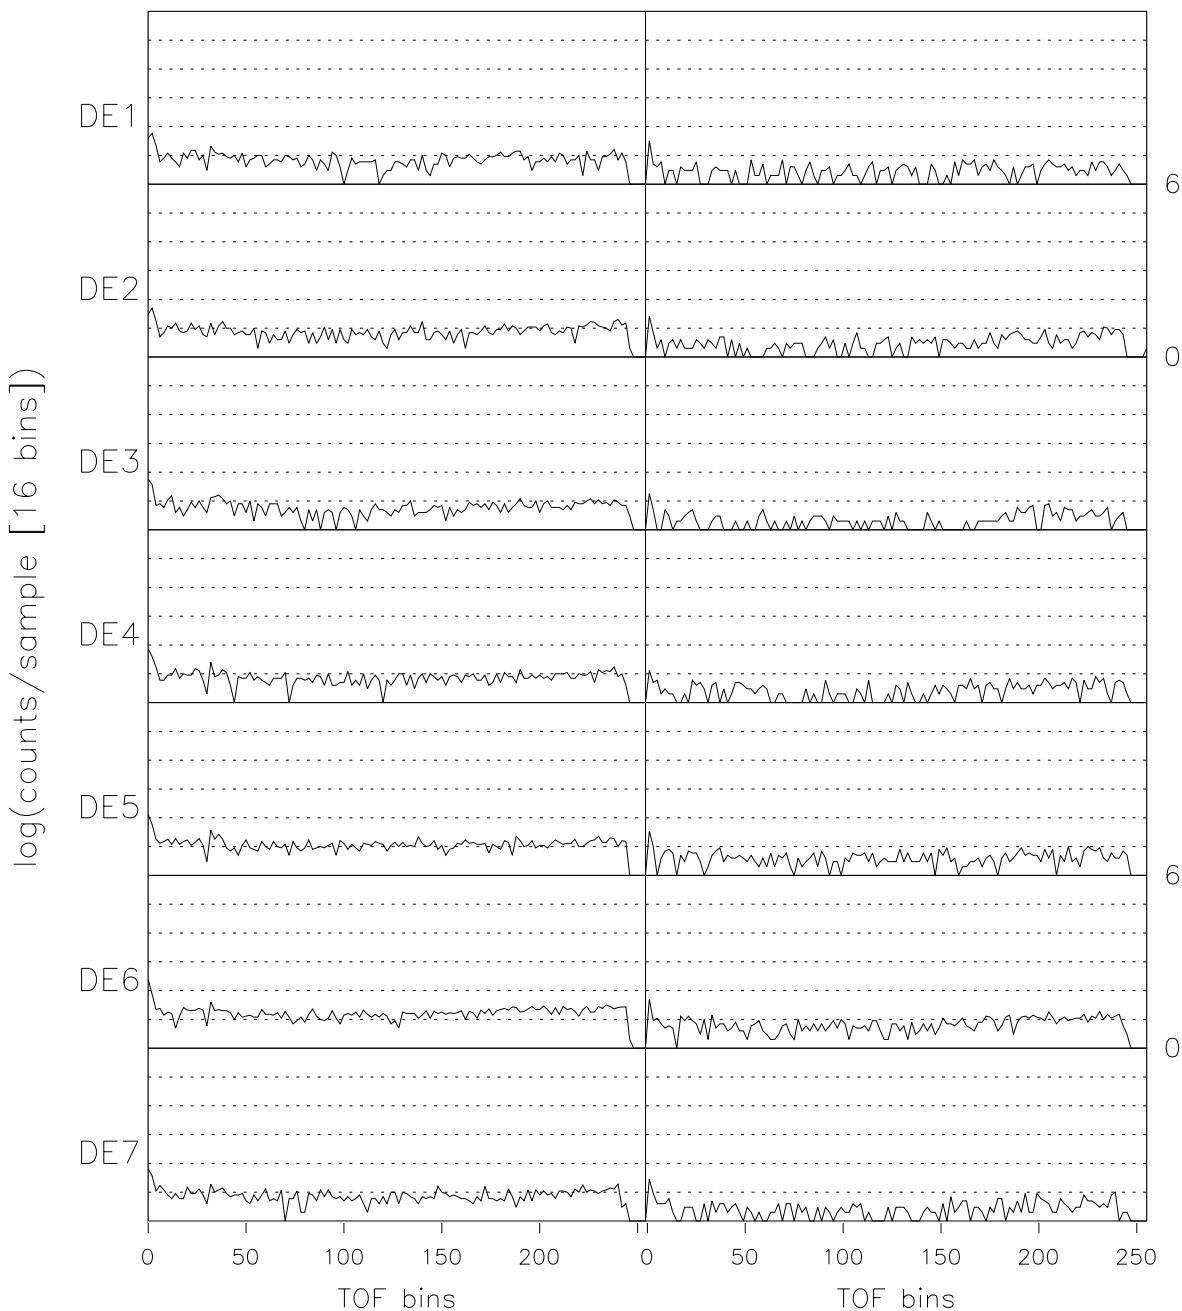

reported: 11-23-06 08:14:08 UT

reported: 11-23-06 08:17:20 UT

file: /export/data/tide/nrt/06112301.dat

-15kV TOF: -9181 v

-3.6kV MCP: -3379 v

-2.4kV MCP: -1774 v

Input Cur: 312 ma

RPA max: 237 v

Mirror max: 238 v